

# Dimensional changes of commercial and novel polyvinyl siloxane impression materials following sodium hypochlorite disinfection (#64727)

1

First submission

## Guidance from your Editor

Please submit by **7 Oct 2021** for the benefit of the authors (and your \$200 publishing discount) .



### Structure and Criteria

Please read the 'Structure and Criteria' page for general guidance.



### Raw data check

Review the raw data.



### Image check

Check that figures and images have not been inappropriately manipulated.

Privacy reminder: If uploading an annotated PDF, remove identifiable information to remain anonymous.

## Files

Download and review all files from the [materials page](#).

2 Figure file(s)

1 Table file(s)

1 Raw data file(s)



# Structure and Criteria

## Structure your review

The review form is divided into 5 sections. Please consider these when composing your review:

1. BASIC REPORTING
2. EXPERIMENTAL DESIGN
3. VALIDITY OF THE FINDINGS
4. General comments
5. Confidential notes to the editor

 You can also annotate this PDF and upload it as part of your review

When ready [submit online](#).

## Editorial Criteria

Use these criteria points to structure your review. The full detailed editorial criteria is on your [guidance page](#).

### BASIC REPORTING

-  Clear, unambiguous, professional English language used throughout.
-  Intro & background to show context. Literature well referenced & relevant.
-  Structure conforms to [PeerJ standards](#), discipline norm, or improved for clarity.
-  Figures are relevant, high quality, well labelled & described.
-  Raw data supplied (see [PeerJ policy](#)).

### EXPERIMENTAL DESIGN

-  Original primary research within [Scope of the journal](#).
-  Research question well defined, relevant & meaningful. It is stated how the research fills an identified knowledge gap.
-  Rigorous investigation performed to a high technical & ethical standard.
-  Methods described with sufficient detail & information to replicate.

### VALIDITY OF THE FINDINGS

-  Impact and novelty not assessed. *Meaningful* replication encouraged where rationale & benefit to literature is clearly stated.
-  All underlying data have been provided; they are robust, statistically sound, & controlled.
-  Conclusions are well stated, linked to original research question & limited to supporting results.



The best reviewers use these techniques

## Tip

## Example

**Support criticisms with evidence from the text or from other sources**

*Smith et al (J of Methodology, 2005, V3, pp 123) have shown that the analysis you use in Lines 241-250 is not the most appropriate for this situation. Please explain why you used this method.*

**Give specific suggestions on how to improve the manuscript**

*Your introduction needs more detail. I suggest that you improve the description at lines 57- 86 to provide more justification for your study (specifically, you should expand upon the knowledge gap being filled).*

**Comment on language and grammar issues**

*The English language should be improved to ensure that an international audience can clearly understand your text. Some examples where the language could be improved include lines 23, 77, 121, 128 – the current phrasing makes comprehension difficult. I suggest you have a colleague who is proficient in English and familiar with the subject matter review your manuscript, or contact a professional editing service.*

**Organize by importance of the issues, and number your points**

1. Your most important issue
2. The next most important item
3. ...
4. The least important points

**Please provide constructive criticism, and avoid personal opinions**

*I thank you for providing the raw data, however your supplemental files need more descriptive metadata identifiers to be useful to future readers. Although your results are compelling, the data analysis should be improved in the following ways: AA, BB, CC*

**Comment on strengths (as well as weaknesses) of the manuscript**

*I commend the authors for their extensive data set, compiled over many years of detailed fieldwork. In addition, the manuscript is clearly written in professional, unambiguous language. If there is a weakness, it is in the statistical analysis (as I have noted above) which should be improved upon before Acceptance.*

# Dimensional changes of commercial and novel polyvinyl siloxane impression materials following sodium hypochlorite disinfection

Shahab Ud Din<sup>Corresp., 1</sup>, Muhammad Sajid<sup>2</sup>, Asfia Saeed<sup>2</sup>, Farooq Ahmad Chaudhary<sup>1</sup>, Mohammad Khursheed Alam<sup>3</sup>, Juneda Sarfraz<sup>1</sup>, Mangala Patel<sup>4</sup>

<sup>1</sup> School of Dentistry (SOD), Federal Medical Teaching Institution (FMTI)/PIMS, Shaheed Zulfiqar Ali Bhutto Medical University (SZABMU), Islamabad, Pakistan

<sup>2</sup> Department of Dental Materials, Islamabad Medical & Dental College, Islamabad, Pakistan

<sup>3</sup> Preventive Dentistry Department, College of Dentistry, Jouf University, 72345, Sakaka, Saudi Arabia

<sup>4</sup> Centre for Oral Bioengineering (Dental Physical Sciences Unit), Bart's and The London School of Medicine and Dentistry, Queen Mary University of London, London, United Kingdom

Corresponding Author: Shahab Ud Din  
Email address: drshahab728@hotmail.com

**Background:** Dental impressions are used to record anatomy of teeth and surrounding oral structures. Impression materials are soiled with saliva and blood leading to cross-contamination. Disinfection reduces cross infection but may have negative impact on dimensional stability of materials. **Objective:** Comparatively evaluate linear dimensional changes of synthesized Tetra-functional (dimethylsilyl) orthosilicate (TFDMOS) containing Polyvinylsiloxane (PVS) impressions following sodium hypochlorite disinfection. **Methods:** Percentage dimensional changes of three commercial PVS (Elite HD Monophase, Extrude and AquaSil Ultra Monophase) and five experimental PVS impression materials were measured. Exp-A (without TFDMOS), Exp-B (with TFDMOS), Exp-C (TFDMOS+ 2% Rhodasurf CET-2), Exp-D (TFDMOS+ 2.5% Rhodasurf CET-2) Exp-E (TFDMOS+ 3% Rhodasurf CET-2) were prepared. Samples were made using rectangular stainless-steel molds (40X10X3 mm<sup>3</sup>) and linear dimensional changes were measured using a calibrated travelling microscope at 10x magnification after immersion in distilled water and 1 % Sodium Hypochlorite solution at 30 minutes and 24 hours. **Results:** Samples immersed in 1% NaOCl showed significant ( $p < 0.05$ ) dimensional changes after 30 minutes of immersion. Exp-E showed significantly greater dimensional changes than their control (Exp-A and Exp-B). In distilled water, there were no significant difference among the tested materials. AquaSil exhibited highest expansion (0.06%) in both solutions. At 24 hours, among the commercial material, extrude had the greatest expansion followed by AquaSil and Elite in DW while AquaSil showed the greatest expansion followed by Extrude and Elite in NaOCl. **Conclusion:** Experimental PVS had linear dimensional changes within ISO 4823; 2015

recommended range. However, extended immersion can negatively affect the linear dimensions.

# **Dimensional changes of commercial and novel polyvinyl siloxane impression materials following sodium hypochlorite disinfection.**

Shahab Ud Din<sup>1</sup>, Muhammad Sajid<sup>2</sup>, Asfia Saeed<sup>2</sup>, Farooq Ahmad Chaudhary <sup>1</sup>, Mohammad Khursheed Alam<sup>3</sup>, Juneda Sarfraz<sup>1</sup>, Mangala Patel<sup>4</sup>

<sup>1</sup> School of Dentistry (SOD), Federal Medical Teaching Institution (FMTI)/PIMS, Shaheed Zulfiqar Ali Bhutto Medical University (SZABMU), Islamabad, Pakistan.

<sup>2</sup> Department of Dental Materials, Islamabad Medical & Dental College, Islamabad, Pakistan.

<sup>3</sup> Preventive Dentistry Department, College of Dentistry, Jouf University, 72345 Sakaka, Saudi Arabia.

<sup>4</sup> Centre for Oral Bioengineering (Dental Physical Sciences Unit), Bart's and The London School of Medicine and Dentistry, Queen Mary University of London, UK.

Corresponding Author:

Shahab Ud Din<sup>1</sup>

School of Dentistry (SOD), Federal Medical Teaching Institution (FMTI)/PIMS, Shaheed Zulfiqar Ali Bhutto Medical University (SZABMU), Islamabad, Pakistan.

Email address: drshahab728@hotmail.com

25

## 26 Abstract

27 **Background:** Dental impressions are used to record anatomy of teeth and surrounding oral  
28 structures. Impression materials are soiled with saliva and blood leading to cross-contamination.  
29 Disinfection reduces cross infection but may have negative impact on dimensional stability of  
30 materials.

31 **Objective:** Comparatively evaluate linear dimensional changes of synthesized Tetra-functional  
32 (dimethylsilyl) orthosilicate (TFDMOS) containing Polyvinylsiloxane (PVS) impressions  
33 following sodium hypochlorite disinfection.

34 **Methods:** Percentage dimensional changes of three commercial PVS (Elite HD Monophase,  
35 Extrude and AquaSil Ultra Monophase) and five experimental PVS impression materials were  
36 measured. Exp-A (without TFDMOS), Exp-B (with TFDMOS), Exp-C (TFDMOS+ 2%  
37 Rhodasurf CET-2), Exp-D (TFDMOS+ 2.5% Rhodasurf CET-2) Exp-E (TFDMOS+ 3%  
38 Rhodasurf CET-2) were prepared. Samples were made using rectangular stainless-steel molds  
39 (40X10X3 mm<sup>3</sup>) and linear dimensional changes were measured using a calibrated travelling  
40 microscope at 10x magnification after immersion in distilled water and 1 % Sodium  
41 Hypochlorite solution at 30 minutes and 24 hours.

42 **Results:** Samples immersed in 1% NaOCl showed significant ( $p<0.05$ ) dimensional changes  
43 after 30 minutes of immersion. Exp-E showed significantly greater dimensional changes than  
44 their control (Exp-A and Exp-B). In distilled water, there were no significant difference among  
45 the tested materials. AquaSil exhibited highest expansion (0.06%) in both solutions. At 24 hours,  
46 among the commercial material, extrude had the greatest expansion followed by AquaSil and

Elite in DW while AquaSil showed the greatest expansion followed by Extrude and Elite in NaOCl.

**Conclusion:** Experimental PVS had linear dimensional changes within ISO 4823; 2015 recommended range. However, extended immersion can negatively affect the linear dimensions.

51

## 52 Introduction

Dental impressions are used to accurately record and reproduce the shape, relationship of teeth and surrounding oral structures (Kumari & Nandeeshwar 2015). However, during impression making, the material becomes soiled with saliva and often with blood which may lead to cross-contamination to the dental team (Ud Din et al. 2018). Different methods of disinfection including spraying and immersion of impression of impression material are commonly employed (Khan 2018). However, American Dental Association (ADA) recommends immersion technique because it allows direct contact of disinfectant solution with all surfaces of the impression (Samra & Bhide 2018).

Among numerous disinfectants available, sodium hypochlorite has been recommended by ADA and Environmental Protection Agency (EPA) for the disinfection of impressions because of its low cost and broad spectrum antimicrobial activity (Correia-Sousa et al. 2013; Khan 2018). Although, disinfection reduces risk of cross infection, alteration in dimensions of impression materials and negative impact on quality of resulting cast has been reported (Guiraldo et al. 2012; Martin et al. 2007). Iwasaki et al. (2016) reported marked change in the dimension of alginate impressions due to water sorption after prolonged immersion of in a disinfectant solution (Iwasaki et al. 2016). Similarly, Babiker et al. (2018) reported significant dimensional



changes of gypsum cast obtained from irreversible hydrocolloids after disinfection by NaOCl immersion (Babiker et al. 2018).

Dimensional stability of the impression materials play a key role in process of constructing a well-fitting prosthesis (Asopa et al. 2020). During recent years, polyvinylsiloxane has gained popularity due to its ability to precisely record tissue details, excellent physical properties and easy manipulation (Azevedo et al. 2019). Nevertheless, these materials have lower tear strength and percentage elongation compared to polysulphide. Additionally, the hydrophobic nature of the material demands a dry field of operation to accurately record fine tissue details (Ud Din et al. 2018). In this context, different researchers have incorporated surfactant to the material composition to synthesized hydrophilic addition silicones, but limited literature is available on methods to improve tear strength of the material (Lee et al. 2004).

Previously, we have synthesized novel TFDMOS containing Polyvinyl siloxane with a non-ionic surfactant (Rhodasurf CET-2) to improve the tear strength and hydrophilicity of conventional addition silicones. It was observed that experimental formulation had significantly higher strength compared to commercially available material and non-ionic surfactant further improved material tear strength (Din et al. 2018). However, considering the variation in material properties corresponding to the composition of the material, the effect of non-ionic surfactant on dimensional stability of material especially after disinfection needed further exploration. It was hypothesized that the experimental formulations have higher water sorption due to presences of non-ionic surfactant, resulting in noticeable dimensional changes.

In addition, the extensive use of polyvinylsiloxane in dentistry and varieties of formulation available demanded a comprehensive comparison of material particularly in terms of dimensional changes following long term disinfection. Therefore, the objective of this study was

two-fold including formulation of experimental polyvinylsiloxane containing TFD MOS and evaluation of the influence of storage media that is distilled water and 1% sodium hypochlorite on the linear dimensional changes over the period of 24 hours, in commercial and synthesized PVS impression materials.

## Materials & Methods

In this study three commercially available medium bodied PVS materials, Aquasil (Ultra, Dentsply, USA), Elite HD Monophase (Zhermack, Italy) and Extrude (Kerr, USA) were selected. In addition, five experimental PVS materials were prepared as base and catalyst paste by weighing all components using four figure balance (Mettler, Toledo Ltd, Model AG204, UK) as already mentioned in published part of the study (Ud Din et al. 2018). The composition of experimental materials is illustrated in Table 1. To prevent premature polymerisation, the prepared material was packed into separate compartments of an auto-mixing cartridge and stored at 4°C. Exp-A served as a control for Exp-B, while Exp-B was used as a control for Exp-C, D and E. Rhodasurf CET-2 (non-ionic surfactant) was incorporated in the base paste of Exp-B at 2, 2.5 and 3% to formulate Exp C, D and E respectively.

A total of eighty samples (n=10) were prepared by introducing the material from automixing syringe into the preformed stainless steel mold (40 x 10 x 2 mm<sup>3</sup>) sandwiched between two metal plates lined by acetate paper. The assembly was placed under a hydraulic press (MESTRA MOD-030350, Talleres Mestraitua, S.L) and the material was allowed to polymerize.

After polymerization, the material was removed from the mold and the specimens (n=5 in each medium) were immersed in 1% NaOCl and distilled water solution for 24 hours at 23 ± 1°C in an

oven (Qualicool incubators, LTE Scientific Ltd). At predetermined time period; which are 10 and 30 min (replicate at-office disinfection), and 60min and 24 hours (simulate the transportation time for the impression to reach the dental laboratory) each sample was removed from the respective liquid, blot dried and linear dimensional changes were recorded using a calibrated travelling microscope (Chesterman, Sheffield, England) by measuring the distance between the fixed edge (secured on a pin) and free end of the sample (movable pin) at 10x magnification. Data was presented as mean and standard deviation using SPSS Version 22 (Armonk NY IBM Corp). Analysis of variance with post hoc Tukey's test was performed to statistically compare all PVS materials at different time points.

## Results

Figure 1 and 2 shows percentage linear dimensional changes of impression materials in DW and 1% NaOCl after 24 hours immersion. AquaSil exhibited highest expansion (0.06%) in both solutions while Exp-A exhibited least expansion (0.01%) in DW. Analysis of variance revealed significant difference ( $p \leq 0.05$ ) in dimensions of tested materials after 30 minutes of immersion in 1% NaOCl. Inter-group analysis revealed statistically similar dimensional changes among all tested materials, except for Exp-E. The surfactant modified Exp-E showed significantly greater dimensional changes than their control groups; Exp-A ( $p=0.003$ ) and Exp-B (0.047). Among commercial materials, although no statistically significant changes in dimensions were observed, AquaSil showed the highest expansion followed by Extrude and Elite in 1% NaOCl solution.



In distilled water, there were no significant difference among the commercial and experimental materials. Extrude had the highest expansion followed by AquaSil and Elite at 24 hours. Exp B showed slightly higher, but statistically similar expansion to Exp-A, while Exp-C, D and E exhibited higher expansion in each immersion solution compared to Exp-B (control) at each interval. Also, expansion of experimental materials was directly related to the concentration of the surfactant

## Discussion

**Add your discussion here.** Impression making is an important aspect of prostheses fabrication. In the oral cavity, these material comes in contact with saliva and blood (Khan 2018). This demands disinfection of materials to prevent cross-infection in dental clinics and hospital. However, it is important that the impressions remain dimensionally stable after disinfection. The results of the present study revealed that immersion of addition silicones impression materials (commercial and experimental) in distilled water does not alter the dimensional stability of the material. On the other hand, expansion of tested materials was noted following disinfection with 1% NaOCl for 24 hours. However, the dimensional changes observed were not clinically relevant as the values are within the permitted range of  $\leq 0.5\%$  as recommended by ISO 4823; 2015 (ISO) and ADA specification 19 (Association 2007). Thus, indicating high precision of the experimental material.

The limited amount of linear expansion could be attributed to the isotropic expansion of the samples as they adhere to the PTFE trough of travelling microscope. These findings were supported by Carvalhal et al (2011) who investigated the dimensional changes of polysulphide, polyether, addition and condensation silicone after immersion disinfection with 0.5% NaOCl and

2% glutaraldehyde. They observed insignificant changes in the linear dimensional of materials and recommended that all synthetic elastomers can be safely disinfected by immersion in 0.5% NaOCl and 2% glutaraldehyde (Carvalho et al. 2011). However, in a similar study, although Samra and Bhide (2018) observed clinically acceptable dimensional changes for alginate and PVS after disinfection with ultraviolet rays and immersion disinfection with sodium hypochlorite, changes in cross-arch space and inter-abutment distance on gypsum cast were noted for materials disinfected by glutaraldehyde immersion (Samra & Bhide 2018).

Furthermore, Exp-E had significantly greater dimensional changes after immersion disinfection with NaOCl. This was in line with a number of studies that indicated hydrophilic silicones have greater tendency to absorb water and expand (Silva & Salvador 2004). Results also indicated that longer immersion periods can affect the materials. These findings were similar to those noted by Johnson (1996), who reported long term dimensional stability of PVS is unsatisfactory (Thouati et al. 1996). Similarly, Kumari and Nandeeshwar (2015) observed significant difference between nondisinfected and disinfected specimen of PVS and polyether after immersion of 16 hours in 0.525% sodium hypochlorite.(Kumari & Nandeeshwar 2015) On contrary, Nassar et al found no statistically significant difference between dimensions of vinyl polyether silicone at time of fabrication and after storage for 1 and 2 weeks in 2.5 % buffered solution of glutaraldehyde and reported that dimensional changes within the material obeyed ANSI/ADA standards (Nassar et al. 2017).

The limitation of this study was that the accuracy of the impression material was determined by studying stability of the impression itself and that the setting expansion of the gypsum cast was not taken in account. However, the results confirmed the high precision of the experimental material, suggesting routine use of these materials for impression of fixed and removable partial

dentures, complete dentures, precision attachments and implants. However, it is suggested to evaluate effect of other disinfectant system.

## Conclusions

All three commercial and five experimental polyvinylsiloxane impressions exhibited linear expansion within the recommended range outlined by ANSI and ISO 4823; 2015 following 24hours of immersion, though extended immersion time amplified dimensional changes within all the groups. Therefore, following disinfection, the silicone impression materials must be poured within twenty-four hours.

## References

- Asopa SJ, Padiyar UN, Verma S, Suri P, Somayaji NS, and Radhakrishnan IC. 2020. Effect of heat sterilization and chemical method of sterilization on the polyvinyl siloxane impression material. A comparative study. *Journal of family medicine and primary care* 9:1348-1353. 10.4103/jfmpc.jfmpc\_1122\_19
- Association ANSIAD. 2007. ANNSI/ADA specification no. 19, dental elastomeric impression materials. Chicago: ADA. *Journal of the American Dental Association* 94:733-741.
- Azevedo MJ, Correia I, Portela A, and Sampaio-Maia B. 2019. A simple and effective method for addition silicone impression disinfection. *The journal of advanced prosthodontics* 11:155-161. 10.4047/jap.2019.11.3.155
- Babiker GH, Nadia Khalifa B, Nasser M, and Alhaji B. 2018. Dimensional accuracy of alginate impressions using different methods of disinfection with varying concentrations. *COMPENDIUM* 39.
- Carvalho C, Mello J, Sobrinho LC, Correr AB, and Sinhoreti M. 2011. Dimensional change of elastomeric materials after immersion in disinfectant solutions for different times. *J Contemp Dent Pract* 12:252-258.
- Correia-Sousa J, Taboia AM, Silva A, Pereira T, Sampaio-Maia B, and Vasconcelos M. 2013. The effect of water and sodium hypochlorite disinfection on alginate impressions. *Revista Portuguesa de Estomatologia, Medicina Dentária e Cirurgia Maxilofacial* 54:8-12.
- Din SU, Parker S, Braden M, and Patel M. 2018. The effects of cross-linking agent and surfactant on the tear strength of novel vinyl polysiloxane impression materials. *Dental materials* 34:e334-e343.

- Guiraldo RD, Borsato TT, Berger SB, Lopes MB, Gonini-Jr A, and Sinhoreti MAC. 2012. Surface detail reproduction and dimensional accuracy of stone models: influence of disinfectant solutions and alginate impression materials. *Brazilian dental journal* 23:417-421.
- ISO E. 4823: 2000-Dentistry: Elastomeric impression materials. *European Committee for Standardization*.
- Iwasaki Y, Hiraguchi H, Iwasaki E, and Yoneyama T. 2016. Effects of immersion disinfection of agar-alginate combined impressions on the surface properties of stone casts. *Dental Materials Journal* 35:45-50.
- Khan MWU. 2018. An overview of dental impression disinfection techniques-a literature review. *JPDA* 27:208.
- Kumari N, and Nandeeshwar D. 2015. The dimensional accuracy of polyvinyl siloxane impression materials using two different impression techniques: An in vitro study. *The Journal of the Indian Prosthodontic Society* 15:211.
- Lee DY, Oh YI, Chung KH, Kim KM, and Kim KN. 2004. Mechanism study on surface activation of surfactant-modified polyvinyl siloxane impression materials. *Journal of applied polymer science* 92:2395-2401.
- Martin N, Martin M, and Jedynakiewicz N. 2007. The dimensional stability of dental impression materials following immersion in disinfecting solutions. *Dental materials* 23:760-768.
- Nassar U, Flores-Mir C, Heo G, and Torrealba Y. 2017. The effect of prolonged storage and disinfection on the dimensional stability of 5 vinyl polyether silicone impression materials. *The journal of advanced prosthodontics* 9:182-187.
- Samra RK, and Bhide SV. 2018. Comparative evaluation of dimensional stability of impression materials from developing countries and developed countries after disinfection with different immersion disinfectant systems and ultraviolet chamber. *The Saudi dental journal* 30:125-141.
- Silva SMLMd, and Salvador MCG. 2004. Effect of the disinfection technique on the linear dimensional stability of dental impression materials. *Journal of Applied Oral Science* 12:244-249.
- Thouati A, Deveau E, lost A, and Behin P. 1996. Dimensional stability of seven elastomeric impression materials immersed in disinfectants. *The Journal of prosthetic dentistry* 76:8-14.
- Ud Din S, Hassan M, Khalid S, Zafar M, Ahmed B, and Patel M. 2018. Effect of surfactant's molecular weight on the wettability of vinyl polysiloxane impression materials after immersion disinfection. *Materials Express* 8:85-92. 10.1166/mex.2018.1413

**Table 1** (on next page)

Composition of Experimental Polyvinyl siloxane impression materials



**Table 1:Composition of Experimental Polyvinyl siloxane impression materials <sup>2</sup>**

Components	Base Paste(Wt %)				
	Exp-A	Exp-B	Exp-C	Exp-D	Exp-E
Vinyl-terminated dimethylpolysiloxane (Mw 62700)	39.90	39.90	37.95	37.46	36.98
Polymethylhydrosiloxane (Mw 2270)	1.10	0.77	0.74	0.73	0.72
Tetra-functional (dimethylsilyl) orthosilicate (Mw 329)	-	0.33	0.32	0.31	0.31
Components	Catalyst Paste(Wt %)				
	Exp-A	Exp-B	Exp-C	Exp-D	Exp-E
Vinyl-terminated dimethylpolysiloxane (Mw 62700)	40.72	40.72	39.51	39.51	39.51
Platinum (0.05 M)	0.06	0.06	1.27	1.27	1.27
Palladium (<1µm)	0.23	0.23	0.22	0.22	0.22
Rhodasurf CET-2	-	-	2.00	2.50	3.00

1

# Figure 1

Mean linear dimensional changes with Standard Deviation of ~~commercial~~ and experimental PVS impression materials over the period of 24 hours following immersion in Distal water

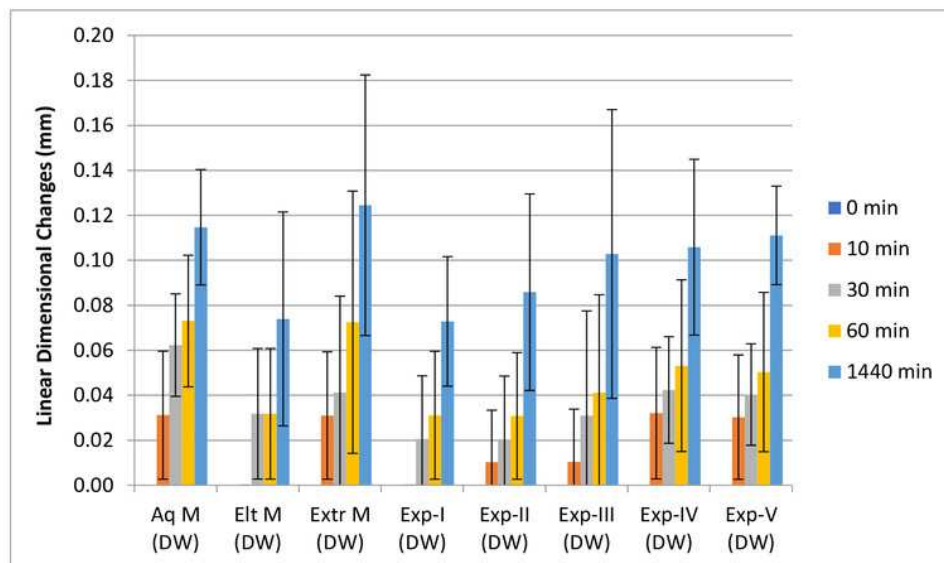


Fig 1: mean linear dimensional changes with Standard Deviation of commercial and experimental PVS impression materials over the period of 24 hours following immersion in Distal water

# Figure 2

Mean linear dimensional changes with Standard Deviation of commercial and experimental PVS impression materials over the period of 24 hours following immersion in 1% NaOCl



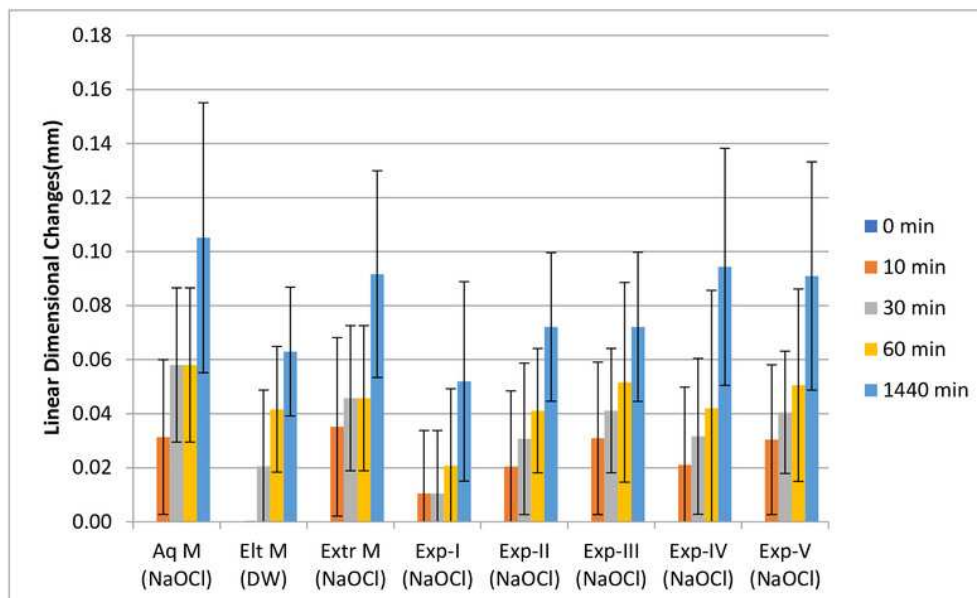


Fig 2: mean linear dimensional changes with Standard Deviation of commercial and experimental PVS impression materials over the period of 24 hours following immersion in 1% NaOCl