



Rapid point-of-care detection of BK virus in urine by an HFman probe-based loop-mediated isothermal amplification assay and a finger-driven microfluidic chip

Yongjuan Zhao^{1,*}, Yi Zeng^{1,*}, Renfei Lu², Zhiying Wang³, Xiaoling Zhang¹, Nannan Wu¹, Tongyu Zhu^{4,5}, Yang Wang³ and Chiyu Zhang¹

¹ Shanghai Public Health Clinical Center, Shanghai, China

² Nantong Third Hospital Affiliated to Nantong University, Nantong, China

³ Beijing Advanced Innovation Center for Biomedical Engineering, Key Laboratory for Biomechanics and Mechanobiology, School of Engineering Medicine, Beihang University, Beijing, China

⁴ Shanghai Medical College, Shanghai, China

⁵ Zhongshan Hospital, Shanghai, China

* These authors contributed equally to this work.

ABSTRACT

Background. BK virus (BKV)-associated nephropathy (BKVN) is one of the leading causes of renal dysfunction and graft loss in renal transplant recipients. Early monitoring of BKV in urine is crucial to minimize the deleterious effects caused by this virus on preservation of graft function.

Methods. We report a simple, rapid, sensitive loop-mediated isothermal amplification (LAMP) assay using an HFman probe for detecting BKV in urine. To evaluate the performance of the assay, a comparison of the HFman probe-based LAMP (HF-LAMP) assay with two qPCR assays was performed using urine samples from 132 HIV-1 infected individuals. We further evaluated the performance of HF-LAMP directly using the urine samples from these HIV-1 infected individuals and 30 kidney transplant recipients without DNA extraction. Furthermore, we combined the HF-LAMP assay with a portable finger-driven microfluidic chip for point-of-care testing (POCT).

Results. The assay has high specificity and sensitivity with a limit of detection (LOD) of 12 copies/reaction and can be completed within 30 min. When the DNA was extracted, the HF-LAMP assay showed an equivalent and potentially even higher sensitivity (93.5%) than the qPCR assays (74.2–87.1%) for 132 urine samples from HIV-1 infected individuals. The HF-LAMP assay can be applied in an extraction-free format and can be completed within 45 min using a simple heat block. Although some decreased performance was seen on urine samples from HIV-1 infected individuals, the sensitivity, specificity, and accuracy of the extraction-free BKV HF-LAMP assay were 95%, 100%, and 96.7% for 30 clinical urine samples from kidney transplant recipients, respectively.

Conclusion. The assay has high specificity and sensitivity. Combined with a portable finger-driven microfluidic chip for easy detection, this method shows great potential for POCT detection of BKV.

Subjects Biotechnology, Molecular Biology, Virology, HIV, BKV

Keywords BK virus, POCT, HF-LAMP, Urine, Finger-driven microfluidic chip

Submitted 11 October 2022

Accepted 1 February 2023

Published 8 March 2023

Corresponding authors

Yang Wang, w_yang89@163.com,

wangyang2022@buaa.edu.cn

Chiyu Zhang,

chiyu_zhang1999@163.com

Academic editor

Srinivas Sistla

Additional Information and
Declarations can be found on
page 13

DOI 10.7717/peerj.14943

© Copyright

2023 Zhao et al.

Distributed under
Creative Commons CC-BY 4.0

OPEN ACCESS

INTRODUCTION

BK virus (BKV), which belongs to the Polyomaviridae family, is a small nonenveloped icosahedral virus with circular doubled-stranded DNA and a genome size of approximately 5,000 bases ([Alcendor, 2019](#)). BKV infects and establishes latency primarily in the urothelium during childhood. BKV is classified into four subtypes (I, II, III, and IV), and subtype I is further subdivided into four subgroups (Ia, Ib1, Ib2, and Ic) based on variation in the VP1 gene sequence ([Hussain et al., 2020](#)). The most common BKV type worldwide is genotype I (approximately 80%), followed by genotype IV (approximately 15%). Up to 80–90% of adults are seropositive for BKV ([Antonsson et al., 2010](#); [Egli et al., 2009](#); [Kamminga et al., 2018](#)). Usually, BKV infection is asymptomatic, but some infections are accompanied by mild respiratory illness or urinary tract disease ([Mischitelli et al., 2008](#)). BKV can establish a persistent infection in the urinary tract ([Furmaga et al., 2022](#)). Latent BKV infection can be reactivated in immunosuppressed individuals and result in related diseases, such as viremia, hemorrhagic cystitis, ureteral stricture, encephalitis, nephritis, retinitis, pneumonia, and even multiple-system organ failure ([Alcendor, 2019](#); [Chong et al., 2019](#)). Most notably, BKV-associated nephropathy (BKVN) is one of the leading causes of renal dysfunction and graft loss in renal transplant recipients. The prevalence of BKVN in renal transplant patients is approximately 10%. Because BKV infection is often asymptomatic at an early stage and there lacks effective antiviral treatments, the risk of graft loss is up to 80% ([Mallavarapu et al., 2021](#); [Teutsch et al., 2015](#)). Currently, the mainstay treatment of BKVN is reduction of immunosuppression ([Teutsch et al., 2015](#)) until the development of specific antiviral treatment strategies. Therefore, the development of a rapid and simple point-of-care testing (POCT) method for the detection of BKV is crucial and necessary to minimize the deleterious effects caused by BKV infection on the preservation of graft function ([Bateman et al., 2017](#); [Gouvea et al., 2016](#)).

Various molecular approaches have been previously developed for the detection of BKV infection. As a gold standard of nucleic acid diagnosis, quantitative polymerase chain reaction (qPCR) is widely used to monitor BKV infection ([Dumoulin & Hirsch, 2011](#); [Hussain et al., 2020](#); [Kato et al., 2017](#)). However, qPCR has some limitations; for example, it requires precise thermal-cycling machines and highly trained personnel, and it is relatively time-consuming (often taking 1–1.5 h), which limit its application for POCT in resource-limited areas. Only approximately 50% of all transplant recipients are evaluated for BK virus infection in resource-limited regions because PCR-based screening assays are expensive and there is limited funding with no medical insurance ([Bagchi et al., 2017](#); [Yooprasert & Rotjanapan, 2018](#)). Hence, a rapid and convenient POCT assay for BKV detection is necessary and will be helpful for decreasing BKVN and transplant complications.

POCT is a promising trend for molecular diagnostics. In particular, the current outbreak of COVID-19 has brought about realization of the necessity and importance of POCT diagnosis, and many nucleic acid POCT methods have been developed ([Augustine et al., 2020](#); [Kang et al., 2022](#)). The loop-mediated isothermal amplification (LAMP) method is a novel nucleic acid amplification method developed in 2000 that uses four primers to

recognize six regions of the target DNA (Notomi *et al.*, 2000). LAMP is capable of detecting even a few copies of a target nucleic acid under isothermal conditions (usually 60–65 °C) using strand-displacing DNA polymerase (Nagamine, Hase & Notomi, 2002; Notomi *et al.*, 2000). Unlike PCR, LAMP can be performed in a low-resource setting using a simple heating device. A LAMP assay using non-sequence-specific fluorescent dye SYBR green was previously developed for BKV detection and showed a sensitivity of 100 copies per reaction (Bista *et al.*, 2007). However, frequent nonspecific amplification largely limit its clinical application. Recently, we developed a multiplexed variant-tolerant real-time LAMP method that utilizes a small amount of additional high-fidelity DNA polymerase to mediate the release of fluorescence signals from a probe (*e.g.*, an HFman probe) (Dong *et al.*, 2022; Zeng *et al.*, 2022). High-fidelity DNA polymerase has a 3′–5′ exonuclease (proofreading) activity to remove 3′-misincorporated nucleotide of newly synthesized DNA or mismatched base in the primer. The use of the HFman probe and high-fidelity DNA polymerase largely improves the specificity of LAMP. Furthermore, this HFman-probe-based LAMP method has comparable performance to qPCR with regard to specificity and sensitivity and a faster reaction speed (approximately 30 min) than the latter (Dong *et al.*, 2022).

In this study, we applied this technique to develop an HFman probe-based LAMP (HF-LAMP) assay for BKV detection. The HF-LAMP assay exhibited high specificity and sensitivity and had very good consistency (98.5%) with the qPCR assay in the detection of 132 HIV-1 infected clinical samples. Furthermore, we further validated the POCT performance of this assay directly using urine (*i.e.*, without DNA extraction) in combination with a portable finger-driven microfluidic chip.

MATERIALS & METHODS

Primer design

Primers and probes specific for the VP1 gene of BKV were designed using Primer Explorer V5 software (Eiken Chemical Co., Ltd., Tokyo, Japan; <https://primerexplorer.jp/e/>) after multiple alignment using MEGA7 (a robust Molecular Evolutionary Genetics Analysis software; <https://www.megasoftware.net/>). Five sets of primers were designed, and each set included two outer primers (F3 and B3), two inner primers (FIP and BIP), and loop primers (LF and/or LB). The primer sequences are shown in Table S1. All primers and probes were synthesized by Sangon Biotech (Shanghai, China).

Preparation of BKV standard

PUC-57 plasmids containing the VP1 gene (GenBank accession no: [AB298947.1](https://www.ncbi.nlm.nih.gov/nuclot/AB298947.1), 1610–2363 nt) of BKV were synthesized by Sangon Biotech (Shanghai, China) as standards. The concentrations of the plasmid standards were quantitated with a Qubit® 4.0 Fluorometer (Thermo Fisher Scientific, Waltham, MA, USA). The copy numbers of the plasmids were calculated using the following formula: $\text{dsDNA copies/mL} = (\text{DNA concentration (g/mL)} / (\text{DNA length} \times 660)) \times 6.022 \times 10^{23}$.

Reaction system of the HF-LAMP assay

The reaction of the HF-LAMP was established according to our previous paper ([Dong et al., 2022](#)). The 25 μ L reaction mixture contains 3 μ L of template, 8 U of Bst 4.0 DNA polymerase (Haigene, Haerbin, China), 0.15 U of Q5[®] high-fidelity DNA polymerase (NEB, Beijing, China), 2.5 μ L of 10 \times Mg²⁺-free isothermal amplification buffer (Haigene, Haerbin, China), 8 mM MgSO₄, 1.8 mM of each dNTP, 0.1 μ M each of F3 and B3, 1.0 μ M each of FIP and BIP, 0.2 μ M LB and 0.2 μ M HFman probe (or LF if used). The reaction was performed at 64 °C for 50 min in a CFX96 Touch Real-Time PCR detection system (Bio-Rad Laboratories, Hercules, CA, USA).

Evaluation of the specificity and sensitivity of the LAMP assay

The specificity of the LAMP system was evaluated using nine common viruses, including human JC polyomavirus (JCV); cytomegalovirus (CMV); papillomavirus types 1, 2, 3, and 4 (HPV-1, HPV-2, HPV-3, HPV-4); hepatitis B virus type 16 (HBV-16); adenoviral type 5 (Adhu5); and human immunodeficiency virus type 1 (HIV-1). Nucleic acids of the nine viruses (50–200 ng/ μ L) were obtained from positive clinical samples. To evaluate the sensitivity of the LAMP system, the BKV standard was ten-fold serially diluted (from 10⁴ to 10⁰ copies/ μ L), and each dilution was used for the reaction.

The limit of detection (LOD) is the lowest detectable concentration at which around 95% of all true positive replicates test positive. To determine the LOD, five-fold serial dilution of the DNA standard (3,000 copies, 600 copies, 120 copies, 24 copies and five copies) were used in the 25 μ L reaction. Each dilution was tested in a set of 20 replicates. The LOD was defined as a 95% probability of obtaining a positive result, using the probit regression analysis implemented in SPSS 17.0 software (SPSS, Inc., Chicago, IL, USA).

Nucleic acid extraction

Nucleic acid was extracted according to the manufacturer's instructions of a commercial BKV qPCR kit (Sinomd Bio, Beijing, China). Fifty microlitres of lysis buffer was added to the precipitates obtained from 1 mL urine samples by centrifugation. The lysate was vortexed and incubated at 65 °C for 30 min. The supernatant was used for nucleic acid detection after centrifugation.

Reaction with a commercial BKV qPCR kit (qPCR assay 1)

Reactions with a commercial BKV qPCR kit (Sinomd Bio, Beijing, China) were performed according to the manufacturer's instructions using a CFX96 Touch Real-Time PCR detection system (Bio-Rad Laboratories, Hercules, CA, USA). Five microlitres of template solution was used for the reaction. The thermal cycling protocol was 1 min at 95 °C for initial denaturation followed by 40 cycles of 5 s at 95 °C for denaturation and 15 s at 60 °C for annealing and extension. The threshold cycle (Ct) of the qPCR assay was determined by the detection system as the cycle at which sample fluorescence crosses the threshold.

In house qPCR assay (qPCR assay 2)

In house qPCR was performed using Premix Ex Taq[™] (Probe qPCR) Kit (Takara Bio Inc. Shiga, Japan) in a CFX96 Touch Real-Time PCR detection system (Bio-Rad Laboratories).

The primer sequences used in the qPCR assay have been described previously ([Leung et al., 2001](#)). The 20 μ L qPCR mixture contained 10 μ L of 2 \times Premix, 1 μ L of 10 μ M BKV forward primer (5'- AGTGGATGGGCAGCCTATGTA-3'), 1 μ L of 10 μ M BKV reverse primer (5'-TCATATCTGGGTCCCCCTGGA-3'), 0.5 μ L of 10 μ M hydrolysis probe (5'-FAM- AGGTAGAAGAGGTTAGGGTGTGTTGATGGCACAG-BHQ1-3'), and 5 μ L of template solution. The thermal cycling protocol was 1 min at 95 °C for initial denaturation followed by 40 cycles of 5 s at 95 °C for denaturation and 15 s at 60 °C for annealing and extension.

Evaluation of BKV HF-LAMP using clinical samples

The clinical sample collection was approved by Shanghai Public Health Clinical Center ethics committee (2018Y032) and registered and recorded at the Chinese Clinical Trial Registry (ChiCTR1800017947). The requirement for informed consent was waived because the clinical urine samples were the rest samples after necessary clinical tests. A total of 132 urine samples from HIV-1 infected individuals were collected at the Clinical Laboratory of the Nantong Third Hospital affiliated with Nantong University Hospital from 2021.9.1 to 2021.9.16. In addition, clinical urine samples from kidney transplant patients were obtained from Shanghai Public Health Clinical Center, including 20 BKV positive samples and 10 BKV negative samples. The status of BKV infection of the kidney transplant patients were previously determined by a digital PCR assay ([Xu et al., 2021](#)). The samples were divided into aliquots and stored at -80°C to avoid frequent freeze-thaw cycles. A commercial BKV qPCR kit (Sinomd Bio, Beijing, China), a reported qPCR assay ([Leung et al., 2001](#)), and HF-LAMP were applied to analyse the urine specimens in parallel. The concordance rate between both assays was calculated with the following formula: (number of consistent results by both methods/total number) $\times 100\%$.

DNA extraction-free HF-LAMP

Fifty microlitres of urine samples collected from HIV-1 infected individuals or kidney transplant patients was incubated at 95 °C for 3 min ([Gandasegui et al. 2015](#)). HF-LAMP was performed directly using 5 μ L of urine. The results were compared with those from the qPCR assay 2. The concordance rate between both assays was calculated with the following formula: (number of consistent results by both methods/total number) $\times 100\%$.

Portable finger-driven microfluidic chip

A portable finger-driven microfluidic chip (Fd-MC) was fabricated according to a previous report with slight modifications ([Wang et al., 2022](#)). The number of reaction chambers was changed from five to two. The volume of waste reservoir been modified for better detection of BK virus from urine samples. Moreover, we integrated the HF-LAMP system in the chip for POCT diagnosis. Integrating with HF-LAMP, 37 urine samples including 27 BKV positive samples and 10 negative samples that were confirmed by the qPCR assay 2, selected from 132 urine samples of HIV-1 infected individuals, and were subjected to the experiments after heating at 95 °C for 3 min by the portable finger-driven microfluidic chip. During manufacturing, the DNA washing buffer (350 μ L) and the LAMP buffer (25 μ L) were pre-packaged into the liquid storage chambers on the substrate. The DNA washing

buffer was 70% ethanol in 10 mM Tris (pH =8), primers and FAM-labeled Hfman probe targeting for the BKV, and RNase-free water (no template control, NTC) were all added to the reaction chambers. LAMP reactions would be initiated once the reaction buffer and the sample containing targets were driven to the sealed chamber by the pressure generated by the finger-actuated operation. Subsequently, the Fd-MC was heated in a water bath at 64 °C for 50 min and the results were read directly by naked eye with an orange filter (Luyor LUV-30A; Luyor, Shanghai, China) under a hand-held blue lamp (Luyor 3260; Luyor, Shanghai, China).

RESULTS

Primer design for the HF-LAMP assay

The VP1 coding region, which is the most conserved genomic region of the virus (GenBank: [AB298947.1](#), 1,610–2,363 bp), shows very high identity (over 95%) in all genotypes of BKV ([Furmaga et al., 2021](#)). Accordingly, LAMP primers were designed to amplify the VP1 gene ([Fig. 1](#)), which is also the target region of most PCR assays ([Xu et al., 2021](#)). For better detection of BKV, five sets of primers were designed based on VP1 gene. To investigate the properties of different sets of primers and thus select the optimal set, all primer sets were subjected to a comparative experiment under the same conditions (reaction system and program, as well as template input). The results indicated that all five sets of primers can be used for amplification of the VP1 gene of BKV ([Fig. S1](#)). Compared to the other four sets of primers, primer set BKV-2 showed higher amplification efficiency with a relatively lower time threshold (Tt) value, which was selected for further use. The primer set BKV-2's information and sequence alignments of the primer and probe regions are shown in [Fig. 1](#) and [Fig. S2](#), respectively.

The HFman probe can be designed with identical sequence to LF or LB. In this study, it was synthesized according to LB sequence, and labelled with a Cy5 fluorophore and a BHQ2 quencher group at the 3'- and 5'-ends (or FAM and BHQ1 at 3'- and 5'-ends), respectively. The 3' fluorescence-labelled base of the HFman probe can be recognized and removed by the high-fidelity DNA polymerase to release fluorescent signal, as previously demonstrated ([Dong et al., 2022](#)).

Specificity and sensitivity of the BKV HF-LAMP assay

The specificity of the BKV HF-LAMP assay was assessed using nine common human viruses, including JCV, CMV, HPV-1, HPV-2, HPV-3, HPV-4, HBV-16, Adhu5, and HIV-1. Except BKV, no amplification curves were observed in any of the other nine common human viruses, indicating a high specificity of the assay ([Fig. 2A](#)). The sensitivity was determined using standards serially diluted 10-fold from 10^4 to 10^3 , 10^2 , 10, and 1 copies/ μ L. Three microlitres of template was added to each LAMP reaction. The detection ability of the LAMP assay was three copies/reaction in less than 20 min ([Fig. 2B](#)). We further measured the LOD of the HF-LAMP assay. The LOD was estimated as 12 copies per 25 μ L reaction and all 20 negative controls were tested at same time without amplification ([Table 1](#)).

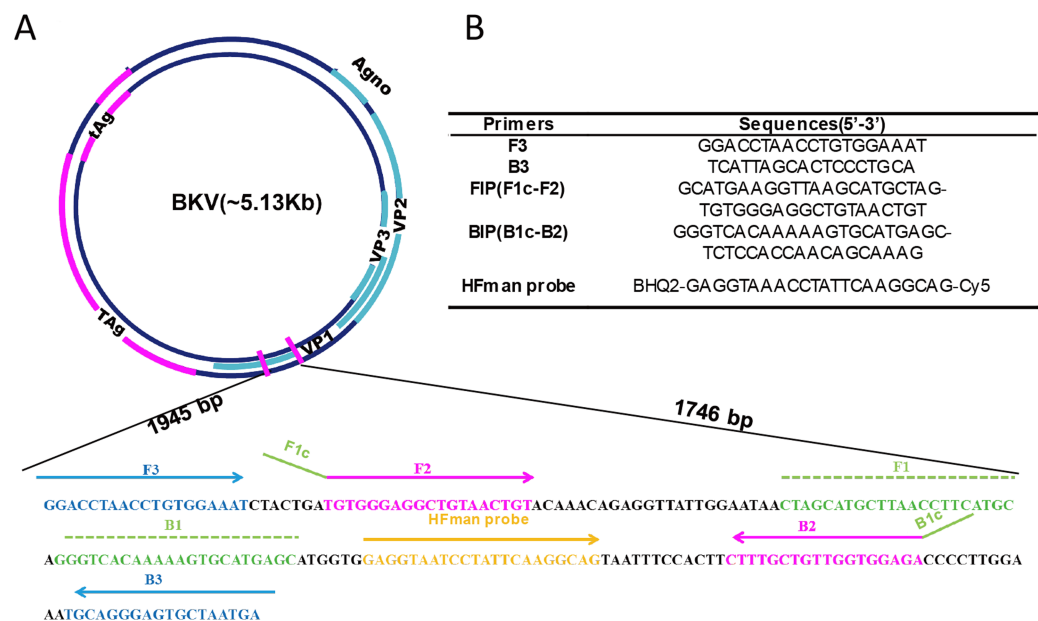


Figure 1 Primer information. Locations (A) and sequences (B) of the primers and probe in the BKV genome. Broad lines indicate open reading frames. Broad purple lines indicate the early region which is predominantly expressed before viral DNA replication to encodes the large T-antigen (T-ag) and small t-antigen (t-ag); broad blue lines indicate the late region which is expressed late in the viral life cycle to encodes the agnoprotein and capsid proteins VP1, VP2, and VP3.

Full-size [DOI: 10.7717/peerj.14943/fig-1](https://doi.org/10.7717/peerj.14943/fig-1)

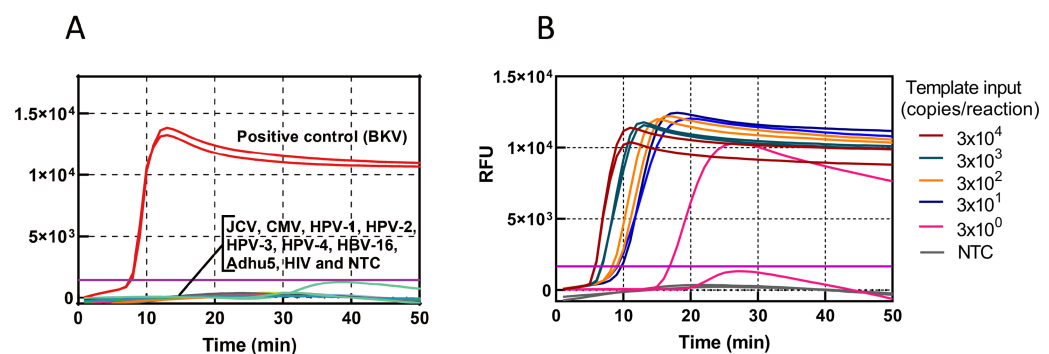


Figure 2 Sensitivity and specificity of the HF-LAMP assay. (A) Specificity of the BKV HF-LAMP assay. Approximately 3000 DNA copies of BKV were used as the positive control. The testing viruses included JCV, CMV, HPV-1, HPV-2, HPV-3, HPV-4, HBV-16, Adhu5, and HIV. (B) Sensitivity of the BKV HF-LAMP assay. The sensitivity of detection was determined with 10-fold serial dilutions of the BKV standard from 3×10^4 to 3×10^0 copies/reaction. NTC: no-template control, purple horizontal line: threshold.

Full-size [DOI: 10.7717/peerj.14943/fig-2](https://doi.org/10.7717/peerj.14943/fig-2)

Evaluation of HF-LAMP using extracted DNA from clinical samples of HIV-1-infected patients

HIV-1 infected individuals are an immune-impaired population and often have a relatively higher BKV-positive rate than other populations (Hu et al., 2018). To verify the clinical

Table 1 Limit of Detection (LOD) of the HF-LAMP for BKV detection.

Template input (copies/25 μ L reaction)	3000	600	120	24	5	LOD (copies/25 μ L reaction)
BKV (positive/total)	20/20	20/20	20/20	20/20	9/20	11.6

Table 2 Comparison of the DNA extraction HF-LAMP assay with two qPCR assays from 132 clinical samples from HIV-1 infected patients.

Method	qPCR assay 1 (commercial qPCR kit, Sinomd)				qPCR assay 2 (previously reported method)			Total	Positive rate (%)
	Items	Pos.	Neg.	Concordance rate (%)	Pos.	Neg.	Concordance rate (%)		
HF-LAMP assay	Pos.	21	8	92.4	27	2	98.5%	29	22.0
	Neg.	2	101		0	103		103	
Total		23	109		27	105		132	
Positive rate (%)			17.4			20.5			

Notes.

Pos., positive; Neg., negative.

applicability of the BKV HF-LAMP assay, a total of 132 urine samples were collected from 132 HIV-1 infected patients. For comparison, an approved commercial qPCR kit (Sinomd Bio, Beijing, China) (qPCR assay 1) and a previously reported qPCR assay (qPCR assay 2) (Leung *et al.*, 2001) were used in parallel. The BKV positive rate among this cohort was 18.9%–22.0% according to the three different assays (Table 2). The BKV positive rate was higher by the HF-LAMP assay (22.0%) than both qPCR assays (18.9% and 20.5%) (Table 2). In particular, all positives by the HF-LAMP assay could be confirmed by at least one qPCR assay. Therefore, two samples that were tested negative by the HF-LAMP assay, were tested positive by the qPCR assay 1 (Fig. 3). If the positive samples by any two of the three assays (or any one of the two qPCR assays) are considered as true positive, the HF-LAMP assay has a higher detection sensitivity (93.5%) than both qPCR assays (74.2% and 87.1%). In addition, the HF-LAMP assay showed a higher concordance rate with the qPCR assay 2 (98.5%, 130/132) than the qPCR assay 1 (Fig. 3B).

The Ct values of both qPCR assays ranged from 16.9 to 36.1 for detected positive samples, while the Tt values of the HF-LAMP assay ranged from 3.9 to 15.4 min (Fig. 3A). In particular, HF-LAMP assay generated positive signals within approximately 15 min for most samples (25/29) (Fig. 3A), while the qPCR assay usually requires at least 1 h for extracted DNA. The results indicate that the LAMP assay was substantially faster than the qPCR assays.

Clinical evaluation of the nucleic acid extraction-free BKV HF-LAMP assay using clinical samples from HIV-1 infected patients

To further simplify the HF-LAMP assay, we developed an easy-to-operate workflow (Fig. 4A) and further evaluated the performance of HF-LAMP directly using HIV-1 infected clinical samples without extraction. The urine was incubated at 95 °C for 3 min

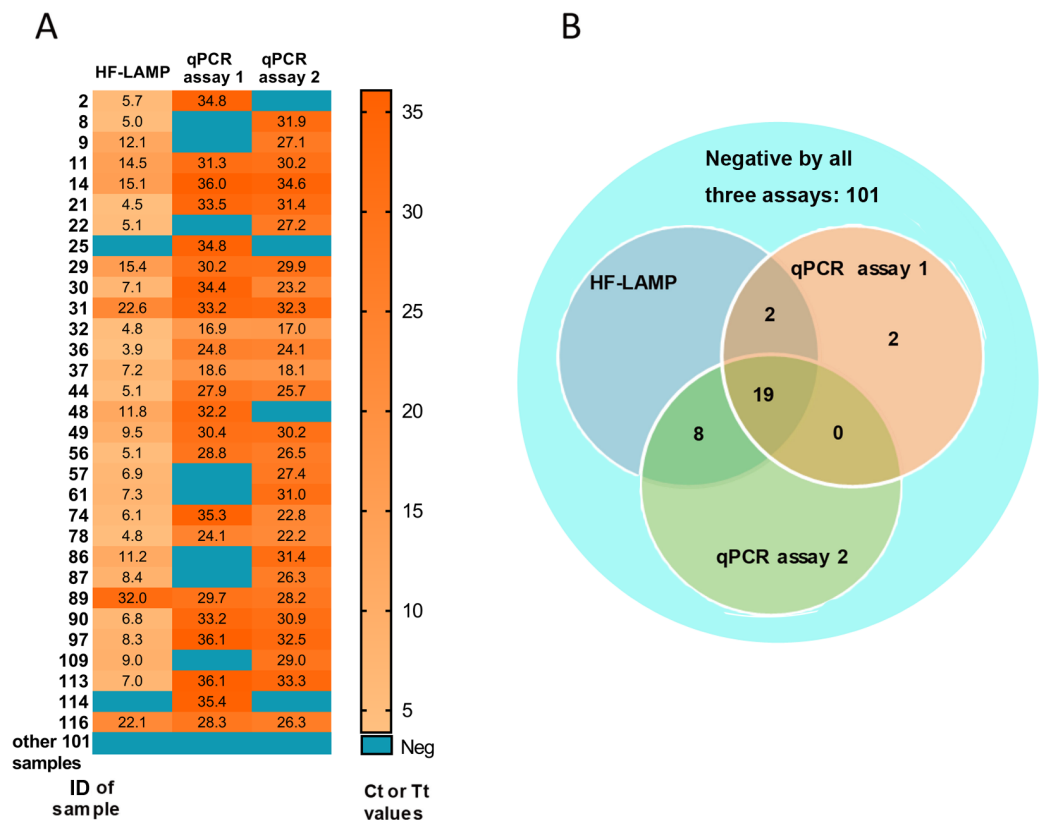


Figure 3 Clinical validation of BKV HF-LAMP using extracted DNA from urine. (A) Heatmap of Tt values of the HF-LAMP assay and Ct values of two qPCR assays on 132 urine samples using extracted DNA. (B) Venn diagram of the number of samples detected by different assays based on the result of qPCR assays 1, the commercial qPCR kit; qPCR assays 2, the previously reported qPCR assay.

Full-size [DOI: 10.7717/peerj.14943/fig-3](https://doi.org/10.7717/peerj.14943/fig-3)

to lyse the viral particles and release nucleic acids. Then, the urine was directly mixed with the LAMP system and placed in the qPCR instrument for amplification (Fig. 4A). Sixteen of 132 urine samples were detected as positive by the extraction-free HF-LAMP assay (Fig. S3). The sensitivity of the extraction-free HF-LAMP assay compared with the reported qPCR assay was 55.5% (15/27). The reasons for relatively low sensitivity may include lower input amounts of samples (compared to those of the reactions with extracted DNA), low viral load in the samples, and the presence of some interfering substances for LAMP. When the Ct values of the samples were less than 25 and 30, the sensitivity of the extraction-free HF-LAMP assay was increased to 100.0% (6/6) and 75.0% (12/16, 95% confidence interval, 0.512–0.988) by SPSS 17.0 software, respectively (Fig. 4B), showing a significantly improved sensitivity. The specificity of the extraction-free HF-LAMP assay was 99.1% (106/107) (Fig. S3).

Clinical evaluation of the nucleic acid extraction-free BKV HF-LAMP assay using clinical samples from kidney transplant patients

To further verify the clinical applicability of the nucleic acid extraction-free BKV HF-LAMP assay, 30 archived clinical urine samples from kidney transplant recipients were tested by

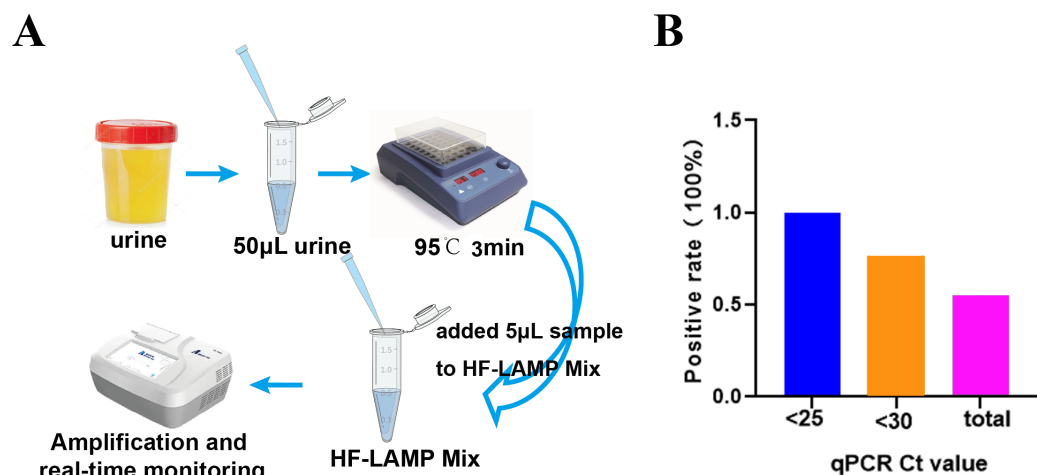


Figure 4 Clinical validation of the DNA extraction-free HF-LAMP method directly using urine samples. (A) Workflow of DNA extraction-free HF-LAMP using urine samples. (B) Positive rate of the extraction-free HF-LAMP assay for all samples and those with Ct values less than 25 and 30 by the qPCR assay 2 (the previously reported qPCR assay) with extracted DNA.

Full-size [DOI: 10.7717/peerj.14943/fig-4](https://doi.org/10.7717/peerj.14943/fig-4)

the extraction-free HF-LAMP assay, the qPCR assay 1 (an approved commercial qPCR kit, (Sinomd Bio, Beijing, China)) and the qPCR assay 2 a previously reported qPCR assay (Leung *et al.*, 2001), in parallel. HF-LAMP, the qPCR assay 1 and qPCR assay 2 detected 19, 19, and 17 out of 20 positive samples previously identified by a digital PCR assay, respectively (Table 2 and Fig. S4). The sensitivity, specificity and accuracy of the extraction-free HF-LAMP assay were 95%, 100%, and 96.7%, respectively, same to those of commercial qPCR kit but slightly higher than previously reported method (Table 3).

POCT detection using a portable finger-driven microfluidic chip

To develop the POCT diagnosis, we further combined the HF-LAMP assay with a portable finger-driven microfluidic chip (Fig. 5) (Wang *et al.*, 2022). An operator-blinded clinical trial was conducted to test 37 HIV-1 infected clinical urine samples, including 27 positive and 10 negative samples, which were confirmed by the previous qPCR assay (qPCR assay 2). The assay achieved a specificity of 80.0% (8/10) and a sensitivity of 74.1% (20/27) based on the 37 clinical samples (Table 4 and Table S2).

DISCUSSION

BKV infection is ubiquitous, and the adult seropositivity rate is estimated to be 80–90% (Antonsson *et al.*, 2010; Egli *et al.*, 2009; Kamminga *et al.*, 2018). BKV infection can cause significant morbidity in immunosuppressed individuals (Replog, Storch & Clifford, 2001). The incidences of BKV viremia and BKVN are 13% and 8% in the kidney transplant recipient population, respectively. In the absence of diagnosis and treatment, BKVN can lead to 80% graft loss (Shen *et al.*, 2021). The 2019 guideline by the American Society of Transplantation Infectious Diseases Community of Practice suggested that all renal transplant recipients should be screened for blood BKV DNA monthly for nine

Table 3 Comparison of the extraction-free HF-LAMP assay with two qPCR assays for 30 clinical samples from kidney transplant patients.

Samples	HF-LAMP assay		qPCR assay 1 (commercial qPCR kit, Sinomd)		qPCR assay 2 (previously reported method)	
	Pos.	Neg.	Pos.	Neg.	Pos.	Neg.
Pos. (<i>n</i> = 20).	19	1	19	1	18	2
Neg. (<i>n</i> = 10)	0	10	0	10	0	10
Total	19	11	19	11	18	12
Sensitivity (%)	95		95		90	
Specificity (%)	100		100		100	
Accuracy (%)	96.7		96.7		93.3	

Notes.
 Pos., positive; Neg., negative.

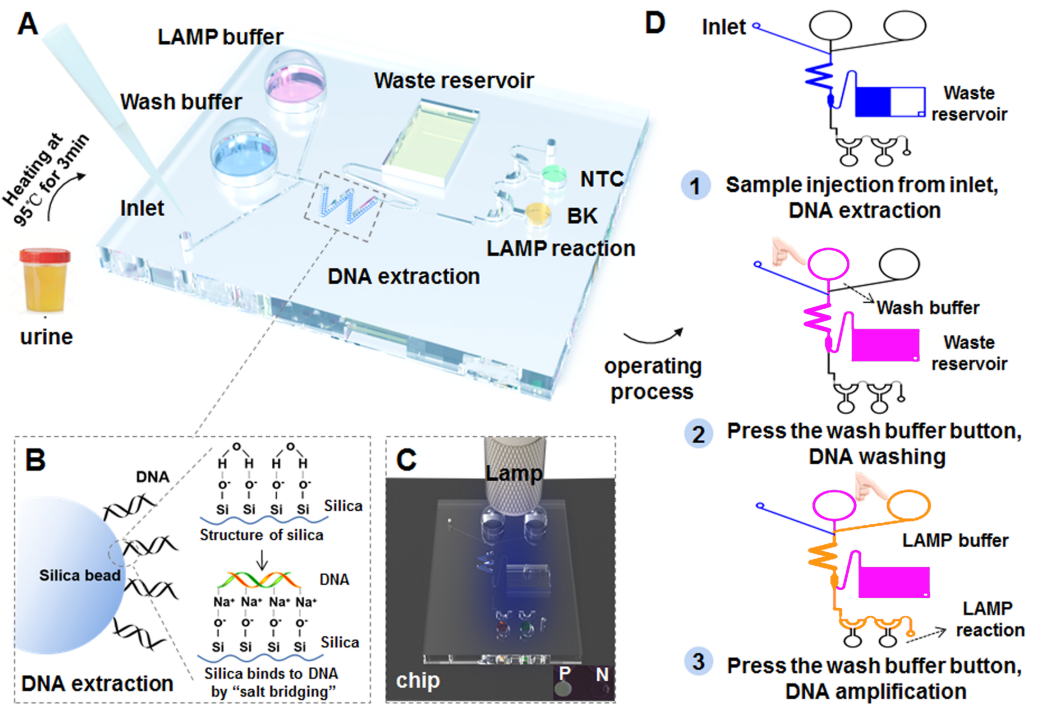


Figure 5 Workflow of the BKV HF-LAMP assay combined with the portable finger-driven microfluidic chip. (A) The structure of the designed finger-driven microfluidic chip; (B) the working principle of the DNA extraction based on silica beads pre-filled into the chip; the wavy blue lines represent surface of silica beads. The figure on the left shows the phenomenon of DNA adsorption, while the figure on the right illustrates the whole principle. (C) The results of the HF-LAMP assay can be read by the fluorescence signal excited by blue lamp light; (D) the operation steps of the BKV detection based on the finger-driven microfluidic chip.

Full-size DOI: 10.7717/peerj.14943/fig-5

Table 4 Comparison of the extraction-free HF-LAMP assay used the portable finger-driven microfluidic chip with qPCR assay 2 for 37 clinical samples from HIV-infected patients.

HF-LAMP assay	qPCR assay 2 (previously reported method)		Total	Positive rate (%)	Concordance rate (%)
	Pos.	Neg.			
Pos.	20	2	22	59.5	75.7
Neg.	7	8	15		
Total	27	10	37		
Positive rate (%)	73.0				

Notes.

Pos., positive; Neg., negative.

consecutive months followed by every 3 months until 2 years post-transplant (*Kidney Disease: Improving Global Outcomes KDIGO Transplant Work Group, 2009*). Therefore, the development of a self-test method for BKV infection is essential for the prevention and control of BKV-associated diseases and deaths.

Although LAMP was developed over 20 years ago (*Notomi et al., 2000*), nonspecific amplification, low detection accuracy, and lack of multiplexing capacity have limited its application. Some efforts were made to mitigate and/or solve these problems and several probe-based LAMP methods were developed. For example, the HFman probe (*Dong et al., 2022*), molecular beacon (*Xu et al., 2022*), assimilating probe (*Lim et al., 2020*), and other strategies (*Ball et al., 2016; Tanner, Zhang & Evans Jr, 2012*) were used in LAMP to achieve specific and multiplex detection. In particular, the HFman probe-based real-time LAMP method (called HF-LAMP) uses a small amount of additional high-fidelity DNA polymerase and an HFman probe in a standard LAMP reaction system not only to achieve specific and multiplex detection but also to improve tolerance to primer-template mismatches caused by various virus variants (*Dong et al., 2022; Xu et al., 2021; Zhang et al., 2022; Zhou et al., 2019; Li et al., 2021*). Therefore, we applied HF-LAMP to develop a POCT assay for BKV infection.

The HF-LAMP assay was first established using extracted DNA. The assay showed a high specificity and sensitivity, and its LOD was 12 copies per 25 μ L reaction. Its performance was further assessed by 132 urine samples from HIV-1 infected individuals. Patient urine and/or blood samples are usually used to detect BKV persistence in kidneys (*Kudose & Dong, 2014*). The direct use of urine as a sample for POCT will enable rapid and noninvasive detection of BKV (*Pinto et al., 2013*). Extracted nucleic acids from clinical samples are usually used in conventional testing workflows, which limits the implementation of POCT and leads to a delay in results. Notably, Bst DNA polymerase has good tolerance to urine components (*Jevtusevskaia et al., 2017*), and thermal lysis is a nucleic acid sample preparation technique without any other processing steps that has been used for urine samples analysis by LAMP (*Gandasegui et al., 2015; Packard et al., 2013*). Therefore, it is feasible for the BKV HF-LAMP assay to be performed with simple heating devices (e.g., dry incubators or water baths), and urine can be directly used to detect the presence of BKV.

Therefore, we further developed the HF-LAMP assay to an extraction-free format, and evaluated its performance directly using clinical urine samples from HIV-1 infected individuals and kidney transplant recipients. BKVN is often associated with a higher BKV load ($>10^7$ copies/mL) in urine ([Hussain et al., 2020](#)). The detection sensitivity (100% for samples with BKV load of $>\sim 10^6$ copies/mL) of the extraction-free HF-LAMP assay enables the early identification in HIV-1 infected individuals with a potential risk of BKVN. For 30 archived clinical urine samples from kidney transplant recipients, the sensitivity, specificity and accuracy of the extraction-free HF-LAMP assay were 95%, 100%, and 96.7%, respectively. It turned out that extraction-free BKV HF-LAMP assay is a promising tool for monitoring BKV infection directly using urine samples. Furthermore, we combined the HF-LAMP assay with a portable finger-driven microfluidic chip to enable a more easy POCT diagnosis of BKV infection ([Wang et al., 2022](#)). Because of a relatively poor performance in sensitivity and specificity, possibly due to a low DNA capture rate of the chip and a weak fluorescence signal of FAM under a hand-held blue lamp, the current version of the portable finger-driven microfluidic chip might not suitable to be a diagnostic method. As a new attempt to POCT detection of BKV, however, the portable finger-driven microfluidic chip can be further improved and optimized in future.

CONCLUSIONS

We developed an HF-LAMP assay for detection of BKV in urine, which shows a comparable specificity and sensitivity to two qPCR assays. Furthermore, an extraction-free format and a portable finger-driven microfluidic chip system of the HF-LAMP assay were developed for easy POCT diagnosis of BKV infection in urine.

ADDITIONAL INFORMATION AND DECLARATIONS

Funding

The study was supported by the Shanghai Science & Technology Innovation Action Program (21Y11900500) and the National Natural Science Foundation of China (81873621). The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

Grant Disclosures

The following grant information was disclosed by the authors:
Shanghai Science & Technology Innovation Action Program: 21Y11900500.
The National Natural Science Foundation of China: 81873621.

Competing Interests

The authors declare there are no competing interests.

Author Contributions

- Yongjuan Zhao performed the experiments, analyzed the data, prepared figures and/or tables, authored or reviewed drafts of the article, and approved the final draft.

- Yi Zeng performed the experiments, prepared figures and/or tables, and approved the final draft.
- Renfei Lu analyzed the data, authored or reviewed drafts of the article, and approved the final draft.
- Zhiying Wang performed the experiments, analyzed the data, prepared figures and/or tables, and approved the final draft.
- Xiaoling Zhang performed the experiments, prepared figures and/or tables, and approved the final draft.
- Nannan Wu analyzed the data, authored or reviewed drafts of the article, and approved the final draft.
- Tongyu Zhu analyzed the data, authored or reviewed drafts of the article, and approved the final draft.
- Yang Wang designed the experiments, supervised the study, analyzed the data, authored or reviewed drafts of the article, and approved the final draft.
- Chiyu Zhang conceived and designed the experiments, supervised the study, analyzed the data, authored or reviewed drafts of the article, and approved the final draft.

Human Ethics

The following information was supplied relating to ethical approvals (i.e., approving body and any reference numbers):

The Shanghai Public Health Clinical Center granted Ethical approval to carry out the study within its facilities (2018Y032) and registered and recorded at the Chinese Clinical Trial Registry (ChiCTR1800017947).

Data Availability

The following information was supplied regarding data availability:

The raw data of LAMP and qPCR are available in the [Supplemental Files](#).

Supplemental Information

Supplemental information for this article can be found online at <http://dx.doi.org/10.7717/peerj.14943#supplemental-information>.

REFERENCES

- Alcendor DJ. 2019.** BK polyomavirus virus glomerular tropism: implications for virus reactivation from latency and amplification during immunosuppression. *Journal of Clinical Medicine* **8**(9):1477 DOI [10.3390/jcm8091477](https://doi.org/10.3390/jcm8091477).
- Antonsson A, Green AC, Mallitt KA, O'Rourke PK, Pawlita M, Waterboer T, Neale RE. 2010.** Prevalence and stability of antibodies to the BK and JC polyomaviruses: a long-term longitudinal study of Australians. *Journal of General Virology* **91**:1849–1853 DOI [10.1099/vir.0.020115-0](https://doi.org/10.1099/vir.0.020115-0).
- Augustine R, Hasan A, Das S, Ahmed R, Mori Y, Notomi T, Kevadiya BD, Thakor AS. 2020.** Loop-mediated isothermal amplification (LAMP): a rapid, sensitive, specific, and cost-effective point-of-care test for coronaviruses in the context of COVID-19 pandemic. *Biology* **9**(8):182 DOI [10.3390/biology9080182](https://doi.org/10.3390/biology9080182).

- Bagchi S, Gopalakrishnan V, Srivastava SK, Upadhyay A, Singh G, Bhowmik D, Mahajan S, Dinda A, Agarwal SK. 2017. BK polyomavirus infection after renal transplantation: surveillance in a resource-challenged setting. *Transplant Infectious Disease* 19(6):e12770 DOI 10.1111/tid.12770.
- Ball CS, Light YK, Koh CY, Wheeler SS, Coffey LL, Meagher RJ. 2016. Quenching of unincorporated amplification signal reporters in reverse-transcription loop-mediated isothermal amplification enabling bright, single-step, closed-tube, and multiplexed detection of RNA viruses. *Analytical Chemistry* 88:3562–3568 DOI 10.1021/acs.analchem.5b04054.
- Bateman AC, Greninger AL, Atienza EE, Limaye AP, Jerome KR, Cook L. 2017. Quantification of BK virus standards by quantitative real-time PCR and droplet digital PCR is confounded by multiple virus populations in the WHO BKV international standard. *Clinical Chemistry* 63:761–769 DOI 10.1373/clinchem.2016.265512.
- Bista BR, Ishwad C, Wadowsky RM, Manna P, Randhawa PS, Gupta G, Adhikari M, Tyagi R, Gasper G, Vats A. 2007. Development of a loop-mediated isothermal amplification assay for rapid detection of BK virus. *Journal of Clinical Microbiology* 45:1581–1587 DOI 10.1128/JCM.01024-06.
- Chong S, Antoni M, Macdonald A, Reeves M, Harber M, Magee CN. 2019. BK virus: current understanding of pathogenicity and clinical disease in transplantation. *Reviews in Medical Virology* 29:e2044 DOI 10.1002/rmv.2044.
- Dong Y, Zhao Y, Li S, Wan Z, Lu R, Yang X, Yu G, Reboud J, Cooper JM, Tian Z, Zhang C. 2022. Multiplex, real-time, point-of-care RT-LAMP for SARS-CoV-2 detection using the HFman probe. *ACS Sensors* 7:730–739 DOI 10.1021/acssensors.1c02079.
- Dumoulin A, Hirsch HH. 2011. Reevaluating and optimizing polyomavirus BK and JC real-time PCR assays to detect rare sequence polymorphisms. *Journal of Clinical Microbiology* 49:1382–1388 DOI 10.1128/JCM.02008-10.
- Egli A, Infanti L, Dumoulin A, Buser A, Samaridis J, Stebler C, Gosert R, Hirsch HH. 2009. Prevalence of polyomavirus BK and JC infection and replication in 400 healthy blood donors. *Journal of Infectious Diseases* 199:837–846 DOI 10.1086/597126.
- Furmaga J, Kowalczyk M, Furmaga O, Rokos CA, Zapolski T, Krakowski L, Jakubczak A, Rudzki S. 2022. Molecular epidemiology and variation of the BK polyomavirus in the population of central and eastern europe based on the example of Poland. *Viruses* 14(2):209 DOI 10.3390/v14020209.
- Furmaga J, Kowalczyk M, Zapolski T, Furmaga O, Krakowski L, Rudzki G, Jaroszynski A, Jakubczak A. 2021. BK polyomavirus-biology, genomic variation and diagnosis. *Viruses* 13(8):1502 DOI 10.3390/v13081502.
- Gandasegui J, Fernandez-Soto P, Carranza-Rodriguez C, Perez-Arellano JL, Vicente B, Lopez-Aban J, Muro A. 2015. The rapid-heat LAMPellet method: a potential diagnostic method for human urogenital schistosomiasis. *PLOS Neglected Tropical Diseases* 9(7):e0003963 DOI 10.1371/journal.pntd.0003963.
- Gouvea AL, Cosendey RI, Carvalho FR, Varella RB, De Souza CF, Lopes PF, Silva AA, Rochael MC, De Moraes HP, Lugon JR, Almeida JR. 2016. Pilot study of early monitoring using urinary screening for BK polyomavirus as a strategy for prevention

- of BKV nephropathy in kidney transplantation. *Transplantation Proceedings* **48**(7):2310–2314 DOI [10.1016/j.transproceed.2016.06.023](https://doi.org/10.1016/j.transproceed.2016.06.023).
- Hu C, Huang Y, Su J, Wang M, Zhou Q, Zhu B. 2018.** The prevalence and isolated subtypes of BK polyomavirus reactivation among patients infected with human immunodeficiency virus-1 in southeastern China. *Archives of Virology* **163**(6):1463–1468 DOI [10.1007/s00705-018-3724-y](https://doi.org/10.1007/s00705-018-3724-y).
- Hussain I, Tasneem F, Gilani US, Arshad MI, Farhan Ul Haque M, Abbas Z, Umer M, Shahzad N. 2020.** Human BK and JC polyomaviruses: molecular insights and prevalence in Asia. *Virus Research* **278**:197860 DOI [10.1016/j.virusres.2020.197860](https://doi.org/10.1016/j.virusres.2020.197860).
- Jevtusevskaja J, Krolov K, Tulp I, Langel U. 2017.** The effect of main urine inhibitors on the activity of different DNA polymerases in loop-mediated isothermal amplification. *Expert Review of Molecular Diagnostics* **17**(4):403–410 DOI [10.1080/14737159.2017.1283218](https://doi.org/10.1080/14737159.2017.1283218).
- Kamminga S, Van der Meijden E, Feltkamp MCW, Zaaijer HL. 2018.** Seroprevalence of fourteen human polyomaviruses determined in blood donors. *PLOS ONE* **13**(10):e0206273 DOI [10.1371/journal.pone.0206273](https://doi.org/10.1371/journal.pone.0206273).
- Kang T, Lu J, Yu T, Long Y, Liu G. 2022.** Advances in nucleic acid amplification techniques (NAATs): COVID-19 point-of-care diagnostics as an example. *Biosensors and Bioelectronics* **206**:114109 DOI [10.1016/j.bios.2022.114109](https://doi.org/10.1016/j.bios.2022.114109).
- Kato J, Mori T, Suzuki T, Ito M, Li TC, Sakurai M, Yamane Y, Yamazaki R, Koda Y, Toyama T, Hasegawa N, Okamoto S. 2017.** Nosocomial BK polyomavirus infection causing hemorrhagic cystitis among patients with hematological malignancies after hematopoietic stem cell transplantation. *American Journal of Transplantation* **17**(9):2428–2433 DOI [10.1111/ajt.14271](https://doi.org/10.1111/ajt.14271).
- Kidney Disease: Improving Global Outcomes (KDIGO) Transplant Work Group. 2009.** KDIGO clinical practice guideline for the care of kidney transplant recipients. *American Journal of Transplantation* **9**(Suppl 3):S1–155 DOI [10.1111/j.1600-6143.2009.02834.x](https://doi.org/10.1111/j.1600-6143.2009.02834.x).
- Kudose S, Dong J. 2014.** Clinical validation study of quantitative real-time PCR assay for detection and monitoring of BK virus nephropathy. *Annals of Clinical and Laboratory Science* **44**(4):455–460.
- Leung AY, Suen CK, Lie AK, Liang RH, Yuen KY, Kwong YL. 2001.** Quantification of polyoma BK viruria in hemorrhagic cystitis complicating bone marrow transplantation. *Blood* **98**:1971–1978 DOI [10.1182/blood.v98.6.1971](https://doi.org/10.1182/blood.v98.6.1971).
- Li Y, Chen X, Zhao Y, Wan Z, Zeng Y, Ma Y, Zhou L, Xu G, Reboud J, Cooper JM, Zhang C. 2021.** A rapid variant-tolerant reverse transcription loop-mediated isothermal amplification assay for the point of care detection of HIV-1. *Analyst* **146**:5347–5356 DOI [10.1039/d1an00598g](https://doi.org/10.1039/d1an00598g).
- Lim DR, Kim HR, Chae HG, Ku BK, Nah JJ, Ryoo S, Wee SH, Lee C, Lyoo YS, Park CK. 2020.** Probe-based real-time reverse transcription loop-mediated isothermal amplification (RRT-LAMP) assay for rapid and specific detection of foot-and-mouth disease virus. *Transboundary and Emerging Diseases* **67**:2936–2945 DOI [10.1111/tbed.13669](https://doi.org/10.1111/tbed.13669).

- Mallavarapu RK, Sanoff SL, Howell DN, Roberts JK. 2021. BK virus nephropathy in non-renal solid organ transplant recipients: are we looking hard enough? *Clinical Transplantation* 35:e14265 DOI 10.1111/ctr.14265.
- Mischitelli M, Bellizzi A, Anzivino E, Fioriti D, Boldorini R, Miglio U, Chiarini F, Di Monaco F, Pietropaolo V. 2008. Complications post renal transplantation: literature focus on BK virus nephropathy and diagnostic tools actually available. *Virology Journal* 5:38 DOI 10.1186/1743-422X-5-38.
- Nagamine K, Hase T, Notomi T. 2002. Accelerated reaction by loop-mediated isothermal amplification using loop primers. *Molecular and Cellular Probes* 16(3):223–229 DOI 10.1006/mcpr.2002.0415.
- Notomi T, Okayama H, Masubuchi H, Yonekawa T, Watanabe K, Amino N, Hase T. 2000. Loop-mediated isothermal amplification of DNA. *Nucleic Acids Research* 28:e63 DOI 10.1093/nar/28.12.e63.
- Packard MM, Wheeler EK, Alocilja EC, Shusteff M. 2013. Performance evaluation of fast microfluidic thermal lysis of bacteria for diagnostic sample preparation. *Diagnostics* 3(1):105–116 DOI 10.3390/diagnostics3010105.
- Pinto GG, Poloni JA, Carneiro LC, Baethgen LF, Barth AL, Pasqualotto AC. 2013. Evaluation of different urine protocols and DNA extraction methods for quantitative detection of BK viruria in kidney transplant patients. *Journal of Virological Methods* 188(12):94–96 DOI 10.1016/j.jviromet.2012.12.006.
- Reploeg MD, Storch GA, Clifford DB. 2001. Bk virus: a clinical review. *Clinical Infectious Diseases* 33:191–202 DOI 10.1086/321813.
- Shen CL, Wu BS, Lien TJ, Yang AH, Yang CY. 2021. BK polyomavirus nephropathy in kidney transplantation: balancing rejection and infection. *Viruses* 13(3):487 DOI 10.3390/v13030487.
- Tanner NA, Zhang Y, Evans Jr TC. 2012. Simultaneous multiple target detection in real-time loop-mediated isothermal amplification. *Biotechniques* 53:81–89 DOI 10.2144/0000113902.
- Teutsch K, Schweitzer F, Knops E, Kaiser R, Pfister H, Verheyen J, Gobel H, Cingoz T, Di Cristanziano V. 2015. Early identification of renal transplant recipients with high risk of polyomavirus-associated nephropathy. *Medical Microbiology and Immunology* 204(6):657–664 DOI 10.1007/s00430-015-0398-x.
- Wang Z, Wang Y, Lin L, Wu T, Zhao Z, Ying B, Chang L. 2022. A finger-driven disposable micro-platform based on isothermal amplification for the application of multiplexed and point-of-care diagnosis of tuberculosis. *Biosensors and Bioelectronics* 195:113663 DOI 10.1016/j.bios.2021.113663.
- Xu L, Qu H, Alonso DG, Yu Z, Yu Y, Shi Y, Hu C, Zhu T, Wu N, Shen F. 2021. Portable integrated digital PCR system for the point-of-care quantification of BK virus from urine samples. *Biosensors and Bioelectronics* 175:112908 DOI 10.1016/j.bios.2020.112908.

- Xu W, Li Q, Xue H, Fei Y, Cui X, Cao M, Xiong X, Xiong X, Yang Y, Wang L. 2022.** Establishment of a rapid method for skipjack tuna (*Katsuwonus pelamis*) authentication using molecular beacons in loop-mediated isothermal amplification. *Food Chemistry* **382**:132365 DOI [10.1016/j.foodchem.2022.132365](https://doi.org/10.1016/j.foodchem.2022.132365).
- Yooprasert P, Rotjanapan P. 2018.** BK virus-associated nephropathy: current situation in a resource-limited country. *Transplantation Proceedings* **50**:130–136 DOI [10.1016/j.transproceed.2017.11.007](https://doi.org/10.1016/j.transproceed.2017.11.007).
- Zeng Y, Feng Y, Zhao Y, Zhang X, Yang L, Wang J, Gao Z, Zhang C. 2022.** An HFman probe-based multiplex reverse transcription loop-mediated isothermal amplification assay for simultaneous detection of hantaan and seoul viruses. *Diagnostics* **12**(8):1925 DOI [10.3390/diagnostics12081925](https://doi.org/10.3390/diagnostics12081925).
- Zhang X, Li H, Liu Z, Zhao Y, Zeng Y, Dong Y, Li L, Zhang C. 2022.** An HFman probe-based reverse transcription loop-mediated isothermal amplification (RT-LAMP) assay for HIV-1 detection. *Molecular and Cellular Probes* **64**:101834 DOI [10.1016/j.mcp.2022.101834](https://doi.org/10.1016/j.mcp.2022.101834).
- Zhou Y, Wan Z, Yang S, Li Y, Li M, Wang B, Hu Y, Xia X, Jin X, Yu N, Zhang C. 2019.** A mismatch-tolerant reverse transcription loop-mediated isothermal amplification method and its application on simultaneous detection of all four serotype of dengue viruses. *Frontiers in Microbiology* **10**:1056 DOI [10.3389/fmicb.2019.01056](https://doi.org/10.3389/fmicb.2019.01056).